



Piezoelectric Accelerometer


PV-91C **NEW**

High-Temperature Resistance CCLD Type




- **High-temperature resistance CCLD type:**
Supports operation in environments up to **170 degrees** centigrade
- **Compact and lightweight design**
minimizes interference with measurement object, ensuring high measurement accuracy

External dimensions

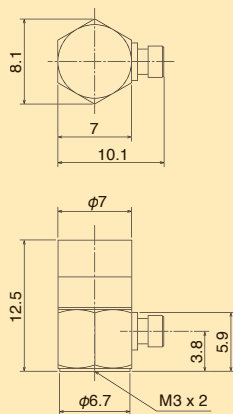

■ Typical frequency response of the PV-91C

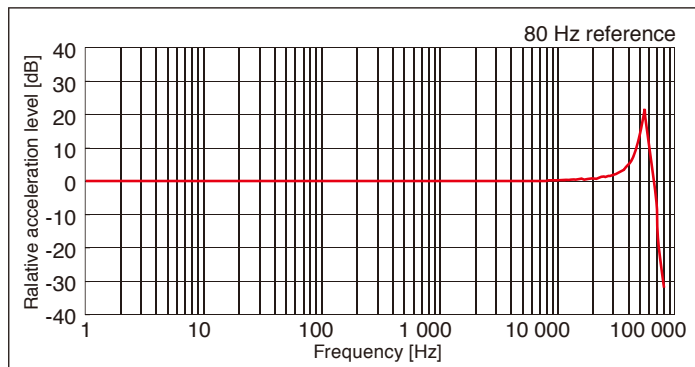

■ Noise Level ACC (Acceleration m/s²) (Typical)

Vibration Meter	VM-83	0.1
Vibration Meter unit	UV-15	0.1
2ch charge amplifier	UV-16	0.1

Specifications

Principle	Shear
Voltage sensitivity (80 Hz) *1	1 mV / (m/s ²) ±15 % (23 °C)
Vibration frequency range Hz *2	1 Hz to 20 kHz (±10 %) from -50 °C to +150 °C 1 Hz to 2 Hz (±15 %) from 150 °C to +170 °C 2 Hz to 20 kHz (±10 %) from 150 °C to +170 °C
Mounting resonance frequency kHz *2	approx. 55 kHz
Maximum measurable acceleration m/s ² (peak) *3	5 000 m/s ² (Peak)
Transverse sensitivity	5 % or less (30 Hz)
Base distortion sensitivity (m/s ²) / μ strain	0.006 (m/s ²) / μ strain (TYP.) (When using 3 Hz high-pass filter)
Thermal transient response (m/s ²) / °C	0.04 (m/s ²) / °C (TYP.) (When using 3 Hz high-pass filter)
Standard mounting method *4	M3 screw 0.5 N·m
Case material	Titanium
Ambient temperature range for operation / °C	-50 °C to +170 °C
Power supply (CCLD)	DC18 V to 30 V (2 mA to 4 mA), rated voltage 24 V
Dimensions	7 mm (Hex) × 12.5 mm (H)
Mass	approx. 1.8 g
Supplied accessories	Ultra-compact accelerometer cable (with ferrite core) VP-51LC (2 m) × 1, M3 screw VP-53K × 2, Insulation attachment VP-53W × 1, Single-head spanner (7 mm) × 1, Hex wrench × 1

Note

- *1 Representative value; actual value is noted on calibration sheet supplied with accelerometer.
- *2 Representative value when mounted on flat surface according to standard mounting method (*4)
- *3 The maximum measurable acceleration differs, depending on temperature, voltage sensitivity, and power supply voltage.

- The piezoelectric element in a piezoelectric accelerometer may be damaged by excessive shock. Take care not to drop the accelerometer, and handle it with care when using the magnetic attachment.

* Specifications subject to change without notice.

Distributed by:

深圳市米乐仪器有限公司
Tel : 0755-28125115
Fax : 0755-28125225
联系人: 李桂乐
<http://www.i1718.com.cn>
E-mail : 361904153@qq.com

This product is environment-friendly. It does not include toxic chemicals on our policy.
This leaflet is printed with environmentally friendly vegetable-based ink on recycled paper.